

Test Report

SL22002294447001TX

Date: September 10, 2020

Page 1 of 3

DONGGUAN YICHANG MEDICAL EQUIPMENT CO.,LTD
BUILDING 1,NO.6,HENGZHONG ROAD,XIN AN,CHANG'AN TOWN,DONGGUAN,GUANGDONG

The following sample(s) was/were submitted and identified on behalf of the client as:

Sample Description : (A) Disposable Vinyl Gloves (SIZE:S)

SGS Internal Ref No. : QDHL2009009170MD

Sample Color : (A) White

Sample Receiving Date : Sep 04, 2020

Testing Period : Sep 04, 2020 - Sep 10, 2020

Test Result(s) : Unless otherwise stated the results shown in this test report refer only to the sample(s) tested, for further details, please refer to the following page(s).

Test Performed : Selected test(s) as requested by applicant

Conclusion	A	Remark
Clause 4.3.2 Determination of pH Value	PASS	
Clause 5.1 Sizing	See Result	
Clause 5.2 Dexterity	See Result	

Remark(s) : PASS=Meet Client's Requirement

Signed for and on behalf of
SGS-CSTC Standards Technical Services (Qingdao) Co., Ltd.

York Yao

York Yao (Account Executive)



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 t (86-532) 6899 9888 f (86-532) 83884258 www.sgs.com.cn
中国·青岛·崂山区株洲路143号通标中心 邮编: 266101 t (86-532) 6899 9888 f (86-532) 83884258 e sgs.china@sgs.com

Test Result

Clause 4.3.2 Determination of pH Value

(ISO 3071:2020; 0.1mol/L KCL extraction)

	Unit	(A)	Requirement
pH Value	-	8.0	3.5-9.5

Note:

- 1) pH value of extraction medium: 5.0 - 7.5
- 2) Temperature of the extraction solution: 22°C

Clause 5.1 Sizing

(EN 420:2003+A1:2009 Clause 6.1)

	1#	2#	Min.
Inner circumference of glove (mm)	180	180	/
Measurements of glove length (mm)	250	251	/
Recommended Size	7		

Remark:

Actual measurements of gloves shall be determined by manufacture, taking into account the behavior of the glove material and intended use. According to Clause 5.1.3, it is possible that the length of gloves designed for special applications may not conform to the values of EN 420:2003+A1:2009 Table 3. For such gloves, the manufacturer shall demonstrate that they are "fit for special purpose" by clearly stating in the instructions for use the intended application(s) and the reason why the gloves do not conform to EN 420:2003+A1:2009 Table 3.

Glove Sizing Requirements

Glove size	Fit		Minimum length of glove (mm)
	Hand size	Hand circumference(mm)	
6	Hands size 6	152	220
7	Hands size 7	178	230
8	Hands size 8	203	240
9	Hands size 9	229	250
10	Hands size 10	254	260
11	Hands size 11	279	270



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 t (86-532) 6899 9888 f (86-532) 83884258 www.sgsgroup.com.cn
 中国·青岛·崂山区株洲路143号通标中心 邮编: 266101 t (86-532) 6899 9888 f (86-532) 83884258 e sgs.china@sgs.com

Clause 5.2 Dexterity

(EN 420:2003+A1:2009, Clause 6.2;)


	Unit	(A)	Requirement
Smallest diameter of pin fulfilling test conditions	mm	5	-
Recommended Level	-	5	-

Remarks:

Finger dexterity test :

- Level 1-Smallest diameter of pin fulfilling test conditions : 11mm
- Level 2-Smallest diameter of pin fulfilling test conditions : 9.5mm
- Level 3-Smallest diameter of pin fulfilling test conditions : 8mm
- Level 4-Smallest diameter of pin fulfilling test conditions : 6.5mm
- Level 5-Smallest diameter of pin fulfilling test conditions : 5mm

Sample Photo

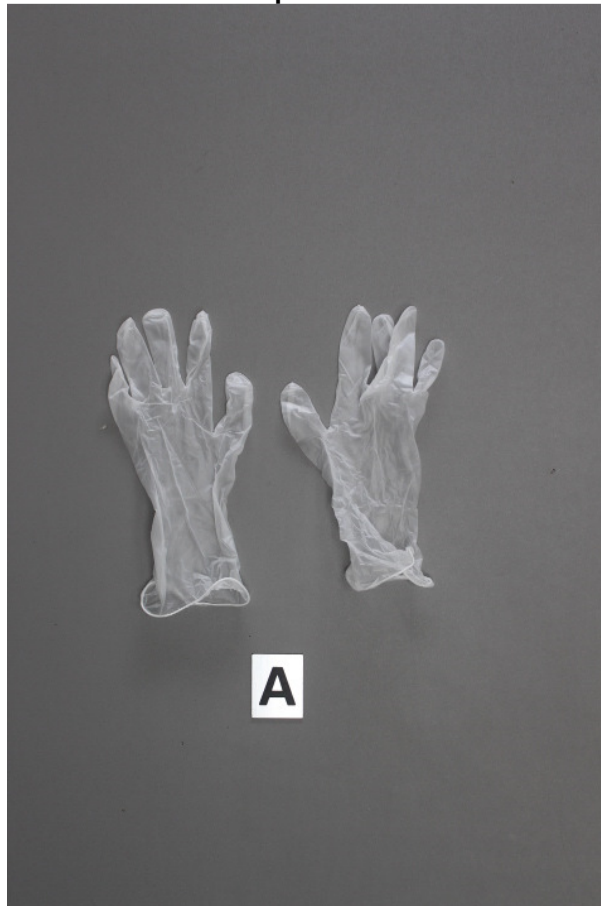

The statement of conformity in this test report is only based on measured values by the laboratory and does not take their uncertainties into consideration.

End of Report



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

SGS Center, No. 143, Zhuzhou Road, Laoshan District, Qingdao, China 266101 t (86-532) 6899 9888 f (86-532) 83884258 www.sgsgroup.com.cn
 中国·青岛·崂山区株洲路143号通标中心 邮编: 266101 t (86-532) 6899 9888 f (86-532) 83884258 e sgs.china@sgs.com